

Mitigating Spectral Errors from White Reference Degradation in Soil Spectroscopy

Simon Ian Futerman¹ , Rachel Lugassi¹, Jonti Evan Shepherd² , Konstantinos Karyotis² , Sabine Chabrilat^{3,4}, Thomas Schmid⁵, José A. M. Demattê⁶ and Eyal Ben Dor¹

Applied Spectroscopy
2026, Vol. 80(2) 155–164
© The Author(s) 2025



Article reuse guidelines:

sagepub.com/journals-permissions

DOI: 10.1177/00037028251396975

journals.sagepub.com/home/asp



Abstract

Soil reflectance spectroscopy is a powerful tool for rapid, non-destructive assessment of soil properties and the foundation for data-driven soil science applications. However, systematic discrepancies during routine spectral measurement procedures, particularly those arising from contamination or deterioration of white reference (WR) calibration panels, may compromise spectral data stability and hinder harmonization practices across laboratories. This study investigates the impact of using a non-contaminated WR panel as a calibration target to measure soil reflectance across the visible (Vis), near-infrared (NIR), and short-wavelength infrared (SWIR) spectral regions. The study evaluates the effectiveness of an internal soil standard (ISS) Lucky Bay sand to correct discrepancies within a controlled laboratory setting. Twelve soils from the Israeli Legacy Soil Spectral Library were analyzed using a contact-probe setup that was calibrated with both a clean and a contaminated WR. The spectral correction method, based on IEEE P4005 protocols and the ISS calibration, significantly reduced spectral inconsistencies, especially in the Vis region where contamination effects were most pronounced. Results show that the ISS effectively harmonized spectra acquired under different WR conditions, reducing the modified average spectral difference stability (mASDS) measure across all samples. While ISS correction is commonly employed for cross-laboratory harmonization, our findings highlight its critical role in enhancing intra-laboratory consistency under routine operational variability. We recommend that every WR calibration process will be accompanied with ISS measurements. The continuous use of a well-maintained WR and ISS improves the reliability of soil spectral datasets and supports the long-term harmonization of soil spectral libraries.

Keywords

Soil spectroscopy, systematic errors, data harmonization, internal soil standard, ISS, white reference, WR

Date received: 10 July 2025; accepted: 21 October 2025

Introduction

Soil spectroscopy has emerged as a transformative tool in soil science, enabling the rapid, non-destructive assessment of a wide range of soil properties.^{1–3} By analyzing soil reflectance across the visible, near-infrared, and shortwave-infrared (Vis-NIR-SWIR) regions (0.35–2.5 μm), it is possible to accurately infer critical physical, chemical, and biological characteristics of soils.^{4–6} This capability supports the development of modern data-driven applications in agriculture, environmental monitoring, and land management, where timely and precise soil information is essential.

Soil spectral libraries (SSLs) are fundamental to these advances. They consist of collections of air-dried soil samples (sieved to <2 mm), paired with both wet chemistry reference data and corresponding spectral measurements.^{7,8} SSLs are critical for developing proximal and remote sensing models which allow for the rapid, non-destructive prediction

¹Remote Sensing Laboratory, Porter School of the Environment and Earth Sciences, Faculty of Exact Sciences, Tel Aviv University, Tel Aviv 699780, Israel

²Aristotle University of Thessaloniki, School of Agriculture, 54124 Thessaloniki, Greece

³Helmholtz Centre for Geosciences GFZ, Remote Sensing and Geoinformatic, Potsdam, Germany

⁴Leibniz University Hannover LUH, Institute of Earth System Science, Soil Science, Germany

⁵Department of Environment, Centro de Investigaciones Energéticas, Medioambientales y Tecnológicas (CIEMAT), 28040 Madrid, Spain

⁶Department of Soil Science, University of São Paulo (USP) 13418-900, Piracicaba, São Paulo, Brazil

Corresponding Author:

Eyal Ben Dor, Remote Sensing Laboratory, Porter School of the Environment and Earth Sciences, Faculty of Exact Sciences, Tel Aviv University, Tel Aviv 699780, Israel.

Email: bandor@tauex.tau.ac.il

of various soil attributes. Soil reflectance spectroscopy captures the interaction of light with soil materials and their chemical chromophores, such as organic matter, iron oxides, clay minerals, and moisture, across the 0.35–2.5 μm Vis-NIR-SWIR range, producing distinctive absorption features that fingerprint key soil properties. Soil reflectance is also influenced by physical chromophores, including particle size distribution, shape, and surface packing, with intercorrelations often occurring between chemical and physical chromophores.^{9–11}

Typically, soil reflectance across the Vis-NIR-SWIR region is measured relative to a standard white reference (WR), often made of materials such as Spectralon, which is characterized by Lambertian properties, spectral featurelessness, and stable high reflectance across the spectral range, calibrated to represent 100% reflectance.^{12–14} Ideally, a calibrated WR is used to ensure accurate absolute reflectance measurements. However, in many practical cases, especially outside controlled laboratory environments, uncalibrated WRs are employed, and only relative reflectance values are recorded.¹⁵

When using soil as a measurement target, WR panels are known to deteriorate both in short and long timescales.^{16–19} In the short term, WR panels can become contaminated by dust, fine soil particles, or micro-scratches, often caused by inadequate cleaning of the panel surface between measurements. Short-term contamination is particularly significant when working with fine soil fractions (<2 mm), which generate dust invisible to the naked eye that cause small particles to adhere to the WR surface via electrostatic forces.²⁰ Additionally, WR ageing effects can occur within several hours of exposure to low levels of irradiance, and their degradation has been shown to continue even when stored in the dark after the exposure.²¹ Over the long term, exposure to environmental conditions, especially outdoor conditions, can gradually degrade their ideal reflectance properties.²² For example, degradation effects were demonstrated with differences of 5% to 23% in wavelengths under 550 nm, between a WR used in field conditions and a pristine, freshly calibrated WR panel.²³ WR panels in soil laboratory settings are typically not absolutely calibrated and are used as relative reflectance references. Even under controlled laboratory conditions, they may degrade over very short periods of time. As a result, reflectance measurements collected in one session may differ from those collected in another, even when taken by the same laboratory using identical procedures.²²

To address systematic errors arising from inconsistencies in soil spectral measurements both in laboratory and field conditions, it was proposed to use an Internal Soil Standard (ISS).²⁴ This approach was later adopted by the IEEE P4005 working group, which is establishing international standards and protocols for soil reflectance measurements across the 0.4–2.5 μm spectral range.²⁵ The ISS reduces systematic variability, allowing harmonization of spectral data across sessions, operators, and even different spectroradiometers, despite minor

procedural differences.²⁶ While the ISS method has demonstrated strong performance across various instruments and protocols,^{1,27,28} its effectiveness in correcting WR degradation within a single laboratory setting over short timeframes, i.e., during one measurement session, has not yet been thoroughly examined. Unlike other systematic effects, such as spectrometer variability or protocol differences, which can be corrected periodically, WR contamination is dynamic and can occur during the measurement process itself, introducing non-systematic errors. Therefore, the WR must be treated as a potential source of systematic error to be controlled and corrected in real time to ensure harmonization. This kind of progressive deterioration provides an ideal scenario to test how the ISS can serve as a stable internal benchmark to support spectral harmonization.

This study presents a detailed assessment of WR panel behavior during routine soil spectral measurements in a single laboratory and aims to examine the use of the ISS for intra-laboratory correction of a contaminated WR. Since WR calibration is a critical step in any soil reflectance protocol, understanding the effects of WR within a single measurement set is essential. We aim to demonstrate best practices for WR maintenance and demonstrate how the ISS can be used to correct measurements taken with a contaminated (dirty) WR, aligning them with those taken using a clean WR.

Experimental

Materials and Methods

Twelve soils from the Israeli Legacy SSL were selected for the study (Figure 1).⁹ These soils were chosen as they vary in their texture, organic matter content (OM), free iron oxides (FED) and carbonates (CaCO_3) and were suitable for examining the effect of calibration with a clean and dirty WR and the subsequent correction with the ISS. They represent common and widespread soil types and include Inceptisol, Mollisol, Entisol, Alfisol, Vertisol, and Aridisol (USDA soil orders). Table 1 provides the soils' chemical and physical data (after Ben Dor and Banin¹¹). The soils were air-dried, gently crushed and sieved to <2 mm. Soil texture was measured using the hydrometer method, OM (%) was determined by the loss-on-ignition method, calcium carbonate (CaCO_3) was determined by the gasometrical method, and FED was determined by dithionite citrate bicarbonate extraction. All references for these traditional wet analyses are provided in Ben Dor et al.⁹ Figure 1 shows the soil samples alongside two WRs from LabSphere (Spectralon, USA): A used (dirty) WR and a seldom-used (clean) WR. Also shown in this figure is the Lucky Bay (LB) ISS (Figure 1).²⁶ Note that typically, laboratories maintain one WR in pristine condition for high-precision measurements (clean), while another WR is used for routine daily work (dirty). The

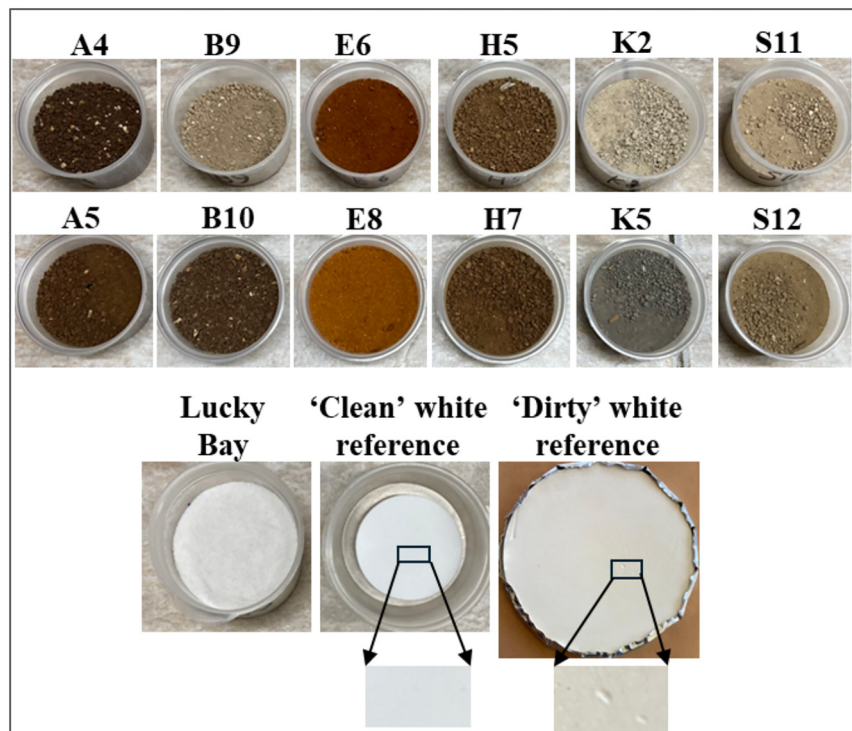


Figure 1. The top two rows are the soils selected for this study and the third row (left to right) is the Lucky Bay (LB) internal soil standard (ISS) used to harmonize the measurements, and a clean and dirty white reference panels used to calibrate the spectrometer.

clean and dirty WR were imaged with a phone camera (iPhone 11) to visually examine their cleanliness.

Soil Spectroscopy Measurements

Soil spectral measurements were acquired using an ASD FieldSpec-4 Hi-Res following the IEEE Standards Association P4005 measurement protocol on air dried <2 mm sieved samples with a contact-probe assembly.²⁵ Prior to any spectral measurement session, the ASD spectrometer was warmed up for 60 minutes as well as the illumination bulb for 30 minutes according to the P4005 protocol. In order to test whether the ISS (Lucky Bay) can correct measurements acquired with a dirty WR compared to a clean WR, two sets of measurements were conducted, each using a different WR panel as a 100% relative reference (clean and dirty). In all measurements a manual elevator was used to bring the sample to the contact probe, to ensure measurement stability. Firstly, the same optimization and calibration was done with the WR for each session (clean and dirty) and the LB ISS measurements along with the soils. The following stages were conducted: (i) Calibration and optimization for WR (clean or dirty), (ii) three-times measurement of LB ISS, (iii) three-times measurement of five soils, and (iv) three-times measurement of LB ISS. Each replication was done by mixing the

soils with a stirrer and preparing the soil surface as homogeneously as possible. The first session was carried out with the clean WR and then the second session used the dirty WR.

Spectral Data Correction Using the ISS

Following both WR sessions (clean and dirty), the LB corrections were applied following²⁹ and the IEEE protocol,²⁵ that was applied to the relative WR (Spectralon) reflectance. The ISS protocol was used to correct the spectral reflectance of all the soils, with the following equation:

$$CF_{\lambda} = 1 - ((Sp_{\lambda} - SBMp_{\lambda}) / Sp_{\lambda}) \quad (1)$$

$$R_{c\lambda} = Ro_{\lambda} * CF_{\lambda} \quad (2)$$

where CF is a correction factor calculated per wavelength, Sp is the reflectance of the local ISS reference (the LB measured at the local user's setup), $SBMp$ is the reflectance of the soil benchmark ISS reference (LB measured at CSIRO-0 setup), which was the spectrum that was acquired at CSIRO using a well calibrated spectrometer against brand new WR from Spectralon), Ro is the original soil sample reflectance (the SOIL spectrum measured at the user's setup), and Rc is the corrected soil sample reflectance (the SOIL spectrum measured at the user's setup normalized to the CSIRO-0 setup).

Table I. The soils used in the study and their properties.

Sample	Soil type (USDA)	Sand (wt%)	Silt (wt%)	Clay (wt%)	CaCO ₃ (%)	Organic matter (%)	Free Fe oxides (%)
A4	Inceptisol	35.1	18.8	46.1	8.46	5.65	1.48
A5	Inceptisol	30.4	15.4	54.2	8.48	2.52	1.60
B10	Mollisol	23.9	16.6	59.5	20.47	2.07	0.99
B9	Entisol	30.1	35.7	34.2	68.34	2.81	0.40
E6	Alfisol	79.6	0.0	20.4	0.63	0.56	0.51
E8	Alfisol	88.6	1.3	10.1	0	0.14	0.25
H5	Vertisol	39.5	14.5	46.0	26.83	2.37	0.84
H7	Vertisol	10.2	24.5	65.3	13.15	2.31	1.15
K2	Aridisol	22.2	38.9	38.9	58.97	2.87	0.28
K5	Aridisol	36.4	25.2	38.4	65.95	2.84	0.07
S11	Entisol	64.2	19.1	16.7	41.79	1.03	0.19
S12	Entisol	74.5	11.4	14.1	21.94	1.93	0.39

Comparing the Spectral Signatures of the Soil Measured with a Clean and Dirty White Reference

Two metrics were used to determine to what extent the LB ISS can correct soil spectra measured with a dirty WR: The modified average spectral difference stability (mASDS); dividing spectra by each other. The mASDS is a widely used metric for assessing the consistency of spectral measurements across all wavelengths. The Calculation of the mASDS is performed as follows:

The mean reflectance at each wavelength across all measurements is calculated as follows:

First, the mean reflectance for each wavelength across all measurements is calculated (mean value between replicates of the same ID for each wavelength, one for the sample measured with a dirty WR, and one for the sample measured with a clean WR) (Eq. 3):

$$S(\lambda) = \frac{1}{n} \sum_{i=1}^n S_i(\lambda) \quad (3)$$

where $S(\lambda)$ is the mean spectral reflectance, λ is a specific wavelength, n is the total number of measurements and $S_i(\lambda)$ is the spectral reflectance of the i th measurements at wavelength (λ).

Next, the absolute difference between the spectral reflectance of each wavelength of each measurement and the mean spectral reflectance (Eq. 3) is calculated (Eq. 4):

$$\Delta S_i(\lambda) = |S_i(\lambda) - S(\lambda)| \quad (4)$$

where $\Delta S_i(\lambda)$ is the absolute difference, $S_i(\lambda)$ is the spectral reflectance of the i th measurement, and $S(\lambda)$ is the mean spectral reflectance for a given wavelength.

Using Eqs. 3–4, the mASDS is calculated and used to quantify the average absolute difference spectral reflectance across all wavelengths and measurements (Eq. 5):

$$\text{mASDS} = \frac{1}{n \cdot m} \sum_{i=1}^n \sum_{\lambda=1}^m \Delta S_i(\lambda) \quad (5)$$

where n is the number of measurements and m is number of wavelengths.

Lower mASDS values indicate a better match between spectra. In this study, we first used mASDS to evaluate the spectral differences between measurements taken with clean and dirty WRs. Then, we applied the LB ISS correction to assess whether it mitigated those differences.

Results and Discussion

From Figure 1, it is apparent that the clean WR is slightly whiter than the dirty WR. Moreover, micro-scratches are also visible on the surface of the dirty WR. Figures 2 and 3 show the soil spectra obtained using both the clean and dirty WR. Visually, the differences between them are minor and not easily detectable to the naked eye. A straight line at 60% is provided to enable better comparison between the two data sets. However, when dividing the spectrum measured with the dirty WR by the spectrum measured with the clean WR (Figure S1, Supplemental Material), the discrepancies become apparent, especially in the visible (Vis) region.

Figure 4 presents the LB ISS measurements obtained with both the dirty and clean WRs, along with the LB measurement provided by CSIRO. It is clearly seen that the dirty WR significantly affects the Vis region, altering its spectral slope.

Figure S2 (Supplemental Material) shows the ratio of LB dirty to LB clean, as well as the ratio between the dirty and clean WRs. These ratios exhibit similar patterns across the Vis region, explaining the discrepancies observed in datasets measured with the different WRs, as highlighted in Figure 3.

Figures 5 and 6 display the soil spectra measured with dirty and clean WRs after applying the LB ISS correction. Spectra discrepancies seem to decrease (in terms of albedo) in both WRs measurements, suggesting that the LB corrected for the shift obtained in the Vis region.

Figure 7 provides examples from two selected soil samples (B9 and B10), each measured with both clean and dirty WRs and then corrected using the LB method. In

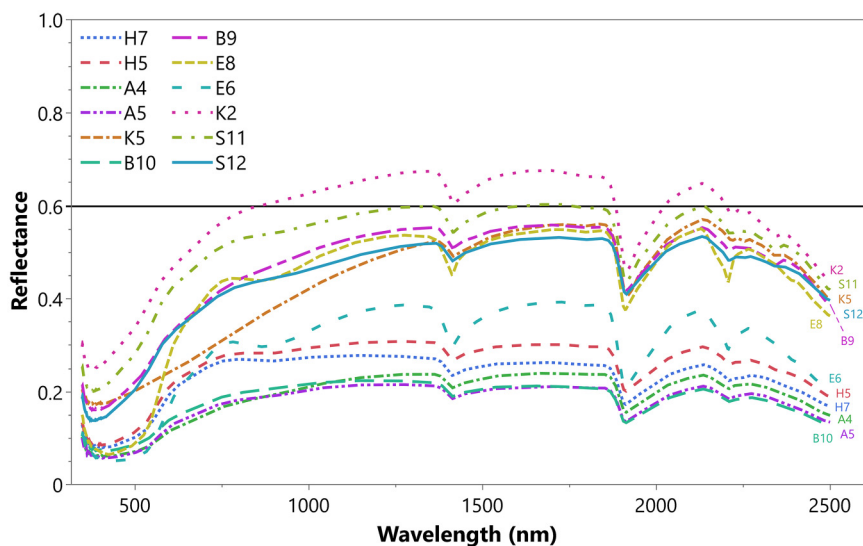


Figure 2. Reflectance of all soils measured with a dirty white reference. The straight line at 0.6 reflectance is a reference to compare changes with Figure 3.

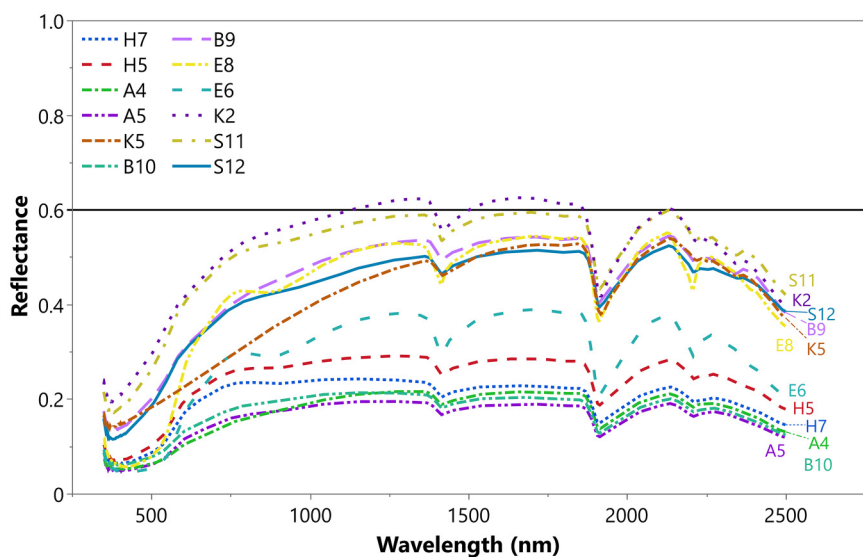


Figure 3. Reflectance of all soils measured with a clean white reference. The straight line at 0.6 reflectance is a reference to compare changes with Figure 2.

both cases, the LB correction effectively reduced the discrepancies introduced by the dirty WVR, resulting in nearly overlapping spectra. To quantify the effectiveness of the LB correction method we used the mASDS metric to demonstrate the effect of the LB correction. mASDS of B9 decreased from 0.008 to 0.001, and that of B10 from 0.004 to 0.002, clearly illustrating the correction’s effectiveness.

To examine the broader effect across the entire sample set, mASDS values were calculated for all samples at each WVR stage (dirty and clean), with and without LB correction. Figure 8 presents the results of this analysis. The correction significantly

improved the spectral consistency in all soils, indicating that the LB ISS correction successfully compensates for contamination in the WVR. Before LB ISS correction, the highest mASDS values were observed in samples K2, H7, K5, A4, and A5 with values of 0.024, 0.015, 0.014, 0.01, and 0.009, respectively. After LB ISS correction, the highest mASDS values were observed in soils K2, H7, A4, K5 and A5 values of 0.018, 0.011, 0.006, 0.005, and 0.005, respectively. Although relatively low compared to values reported in the literature,³⁰ these residual differences may result from other non-systematic effects encountered during measurements.

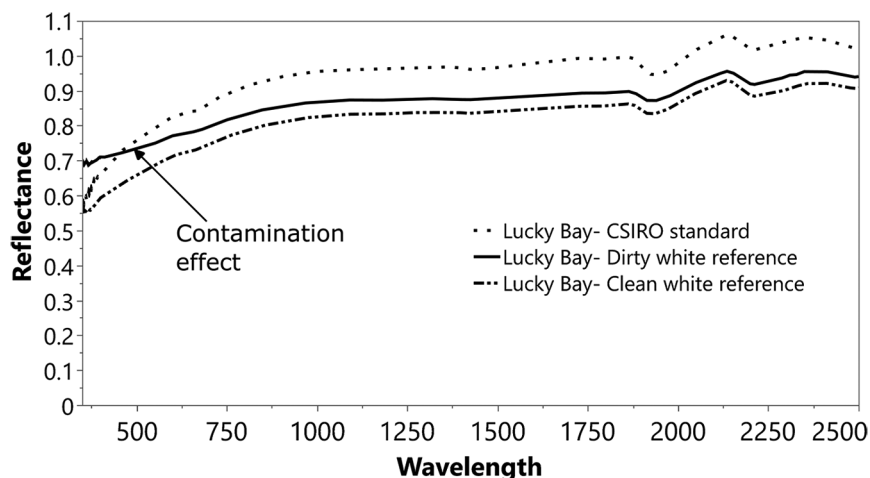


Figure 4. Spectral reflectance of LB ISS. Dotted line: CSIRO standard.²⁹ Solid line: Measured after optimizing and calibrating using the dirty white reference. Dashed line: Measured after optimizing and calibrating using the clean white reference.

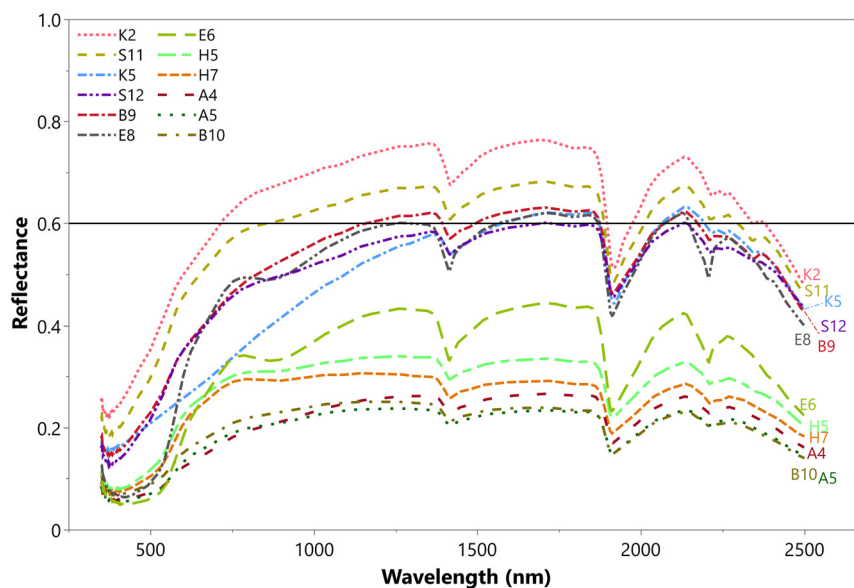


Figure 5. Reflectance of all soils measured relative to a dirty white reference (WR) after ISS LB correction. The straight line at 0.6 reflectance is a reference to compare changes with Figure 6.

In practical laboratory or field settings, the WR can become contaminated, especially after extensive use with numerous soil samples. A major source of contamination can be generated if the sapphire window of the contact-probe assembly is inadequately cleaned between measurements, leading to micro-particles adhering to the assembly, that later contaminate the WR when it is been measured. Indeed, compared to the clean WR, the dirty WR appears contaminated with dust and micro-scratches (Figure 1). Since this contamination often occurs gradually and in the short term, users may not notice the slight brightness change of the WR compared to a clean WR during regular work.²¹ As a result, measurements may be taken

systematically using a non-ideal WR. Short-term WR contamination caused by dust, micro scratches, and even low irradiance, may introduce significant spectral distortions over time, especially in the Vis region of the spectrum which is particularly sensitive to scattering effects (Figures 2 and 3). These results agree with previous studies showing that the Vis regions is especially sensitive to WR deterioration.^{16,21,23} This is particularly concerning because the Vis slope is often used in soil spectroscopy models to estimate properties such as soil organic matter (SOM)³¹ and iron oxides.³² In many cases the minor changes in the WR spectrum used at the same laboratory may not be visible to the naked eye, and therefore if not considered or

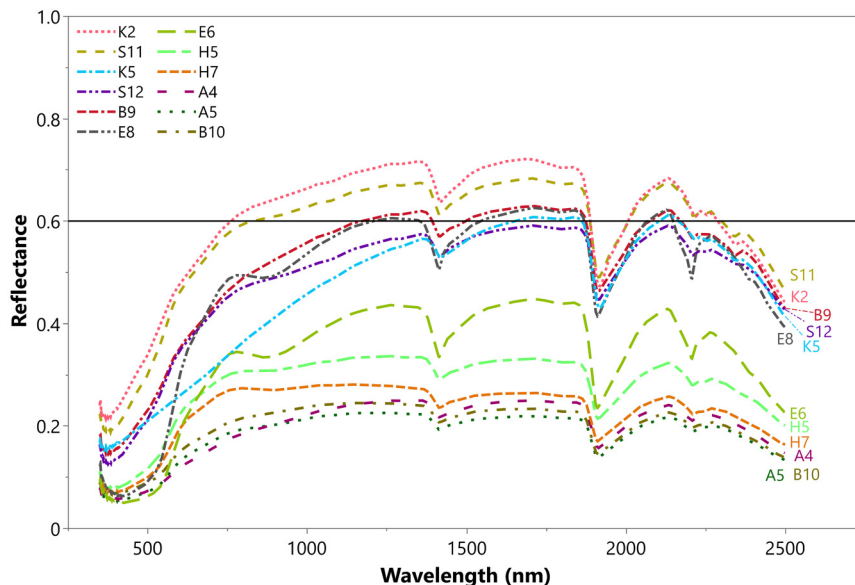


Figure 6. Reflectance of all soils relative to a clean white reference (WR) after ISS LB correction. The straight line at 0.6 reflectance is a reference to compare changes with Figure 5.

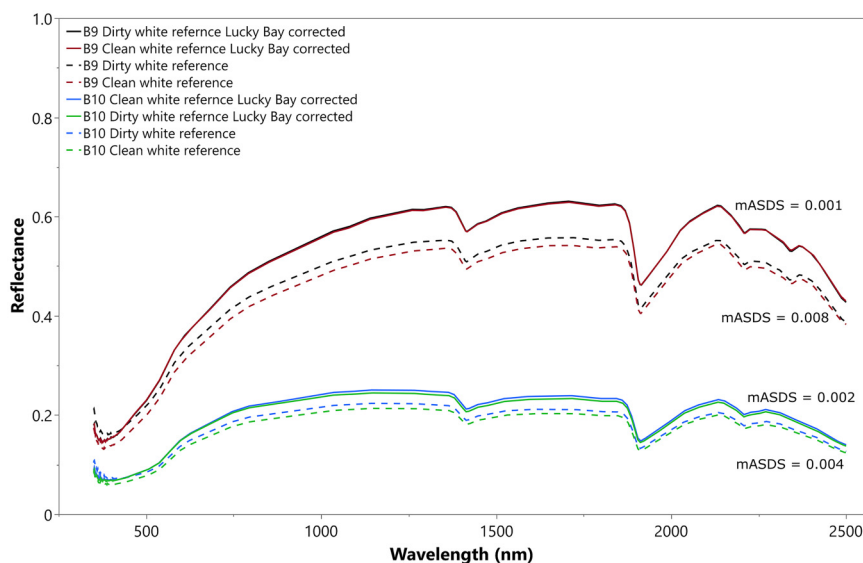


Figure 7. Spectral signatures of two soils (B9 and B10) measured with a clean and dirty white reference, before (dashed lines) and after (full lines) after ISS LB corrections.

corrected, will affect harmonization of measurements from one session to another even within the same laboratory, and consequent downstream data analysis.

To address this issue, using a clean and well-maintained WR is essential. WR maintenance includes storage in a clean, dust-free case and in a clean environment when not in use. Lightly soiled panels can be air brushed with a jet of clean dry air or nitrogen. Heavily soiled WR panels should be restored before use, following existing protocols.³³ During lab or field work,

WR exposure to direct contact with soil, vegetation, moisture, and oily substances should be minimized. A practical suggestion to avoid WR contamination is to have a dual WR setup: one very clean (and if possible, absolutely calibrated) WR, and another one as the WR used in routine measurements. From time to time a spectral measurement of both WRs should be taken. Then, a transfer function should be calculated between the two WRs to ensure that the WR used in routine measurements is aligned with the clean, calibrated WR. However, even

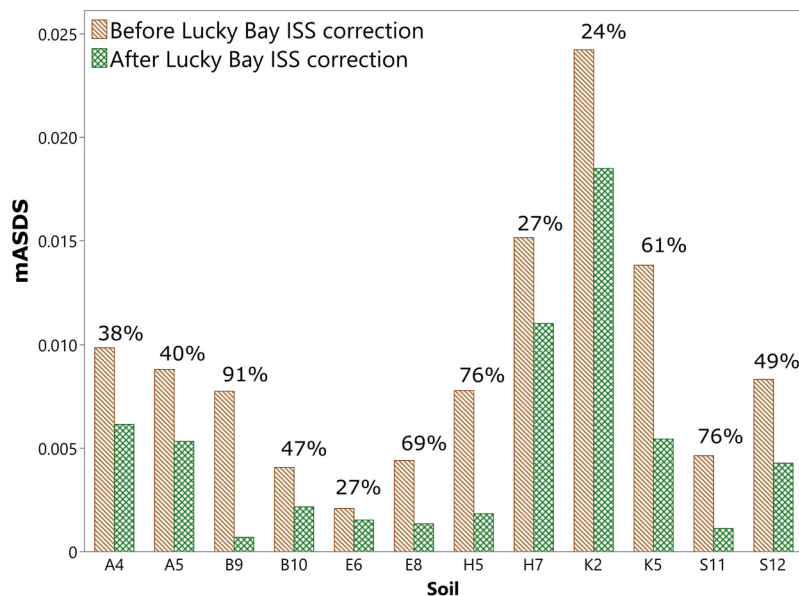


Figure 8. Modified average spectral difference stability (mASDS) of soil spectral reflectance before and after performing ISS LB corrections. Numbers above bars represent the percent of differences of the mASDS before and after LB ISS correction.

with these precautions the WR still deteriorates and gets contaminated over time. As such, using a properly maintained ISS, can serve as an additional correction reference during measurements. The ISS correction method is conducted utilizing the standard LB ISS spectrum, which was measured with a calibrated, clean WR at CSIRO, and is available to all users (Figure 4).²⁹ The LB ISS correction reduced mASDS values across all soils measured in this study (Figures 5 and 6), demonstrating its effectiveness to correct, to some extent, the effects of using a dirty WR (Figures 7 and 8). Although the correction was effective in all soils, it should be noted that in some soils the correction performed better than in others (Figure 8). This may be explained by the soils' inherent properties such as texture, CaCO₃, and organic matter, Fe or other properties, or by a combination of several properties. The original paper introducing the LB ISS showed similar results, with corrections ranging from 20% to 89%.²⁹ Further research could be conducted to more explicitly find the underlying reasons and the most important soil properties that affect the LB ISS correction performance.

The advantage of using an ISS is that it is systematically included in every measurement session (measured before and after every five soils), allowing it to mitigate the effects of minor WR contamination and serve as a transfer standard to a reference (benchmark) laboratory. Unlike occasional recalibration practices, where a correction factor is estimated intermittently between a clean and working WR, the continuous use of the ISS, especially after each WR measurement, ensures systematic and repeatable correction.²⁵ WR contamination can lead to inconsistencies within a single lab, as shown here, and also when harmonizing spectral datasets collected across different laboratories using WR in varying conditions. This makes the use of a clean WR and the use

of the ISS even more critical for ensuring cross-laboratory comparability, especially as soil spectral libraries are being developed and expanded globally.^{8,34,35} Assuming that the white reference (WR) panel deteriorates over both short and long timescales, it is essential to evaluate its spectral characteristics during every measurement session. The ISS may also help correct other systematic effects, such as instrument drift or operational inconsistencies. While measurement protocols are designed to minimize non-systematic errors,²⁴ such effects can still occur occasionally and should not be ignored.

The LB ISS sample itself may accumulate some contamination during lab measurements. In such cases, it is reasonable to assume that the contamination is negligible compared to that of the WR. In addition, if a severe contamination occurs within the LB sample, it is assumed that this effect will be consistent within each measurement session, introducing a systematic bias that can be corrected with the ISS correction. A practical solution to avoid LB contamination may be to split the LB sample into clean and working LB and from time to time to measure them both and generate a transfer function from the working LB to the clean LB. In the case of field work, it is impractical to use the LB sample itself in field settings, as it may become easily contaminated in field settings and relatively large amounts of LB would be required. Hence, for field work, it was recently suggested to select a soil (sand dune) that can be used as an ISS, that bridges the gap between field and lab work.³⁶ They term it a field ISS (FISS) and suggest correcting its' reflectance to the LB ISS with a transfer function, thus creating a pseudo-LB for field work. As WR contamination in field settings can readily occur, using a FISS could alleviate, to some extent, the effect

of a dirty WR in field settings, as shown in this study conducted in a lab setting.

In summary, the ISS is an acceptable method to harmonize spectral measurement of soils between laboratories, and its use is essential. The results show that WR contamination primarily affects the Vis region, which if not treated correctly, can significantly alter spectral data and downstream analyses. The use of a consistent ISS, which was well characterized at an agreed benchmark laboratory, is an effective method to correct WR deterioration and ensures data reliability in soil spectroscopy applications.

Conclusion

This study demonstrates that even minor, short-term contamination of a white reference (WR) panel during routine soil spectral measurements can introduce systematic distortions, particularly in the visible region, which may significantly affect the accuracy of spectral models, especially those estimating soil organic matter. Although such distortions are often visually imperceptible, they can accumulate quickly and compromise data reliability.

The Internal Soil Standard (ISS) from the Lucky Bay site proved highly effective in correcting these distortions, successfully harmonizing spectra measured with both clean and contaminated WRs. The ISS correction notably reduced the modified average spectral difference stability (mASDS) across all tested samples, confirming its utility for intra-laboratory harmonization, not just across different laboratories and protocols. Importantly, this study highlights the need to measure the ISS alongside every WR calibration, instead of only at the beginning or end of a session, as WR degradation can occur even between consecutive measurements. Incorporating ISS measurements throughout the process provides a robust means to monitor WR quality and maintain spectral consistency. Overall, the ISS serves as a valuable tool for improving data reliability, enabling consistent soil spectral measurements, and supporting the long-term integrity of soil spectral libraries.

Acknowledgments

This research received financial support from the WHEATWATCHER project, funded through the EU's Horizon Europe program, under Grant Agreement no. 101156480.

We would like to thank the reviewers for their valuable comments.

ORCID iDs

Simon Ian Futerman  <https://orcid.org/0000-0002-3695-1313>
 Jonti Evan Shepherd  <https://orcid.org/0000-0002-8494-4177>
 Konstantinos Karyotis  <https://orcid.org/0000-0003-1190-5772>

Supplemental Material

All supplemental material mentioned in the text is available in the online version of the journal.

References

1. S. Chabrilat, E. Ben-Dor, J. Cierniewski, C. Gomez, et al. "Imaging Spectroscopy for Soil Mapping and Monitoring". *Surv. Geophys.* 2019. 40(3): 361–399. [10.1007/s10712-019-09524-0](https://doi.org/10.1007/s10712-019-09524-0)
2. M. Nocita, A. Stevens, B. van Wesemael, M. Aitkenhead, et al. "Soil Spectroscopy: An Alternative to Wet Chemistry for Soil Monitoring". *Adv. Agron.* 2015. 132: 139–159. [10.1016/bs.agron.2015.02.002](https://doi.org/10.1016/bs.agron.2015.02.002)
3. R.R. Poppiel, A.F. da S. Paiva, J.A.M. Demattê. "Bridging the Gap Between Soil Spectroscopy and Traditional Laboratory: Insights for Routine Implementation". *Geoderma.* 2022. 425: 116029. [10.1016/j.geoderma.2022.116029](https://doi.org/10.1016/j.geoderma.2022.116029)
4. M.-M. Couêteaux, B. Berg, P. Rovira. "Near Infrared Reflectance Spectroscopy for Determination of Organic Matter Fractions Including Microbial Biomass in Coniferous Forest Soils". *Soil Biol. Biochem.* 2003. 35(12): 1587–1600. [10.1016/j.soilbio.2003.08.003](https://doi.org/10.1016/j.soilbio.2003.08.003)
5. J.A.M. Demattê, M.R. Nanni, A.P. da Silva, J.F. de Melo Filho, et al. "Soil Density Evaluated by Spectral Reflectance as an Evidence of Compaction Effects". *Int. J. Remote Sens.* 2010. 31(2): 403–422. [10.1080/01431160902893469](https://doi.org/10.1080/01431160902893469)
6. B. Ludwig, P.K. Khanna, J. Bauhus, P. Hopmans. "Near Infrared Spectroscopy of Forest Soils to Determine Chemical and Biological Properties Related to Soil Sustainability". *For. Ecol. Manag.* 2002. 171(1): 121–132. [10.1016/S0378-1127\(02\)00467-X](https://doi.org/10.1016/S0378-1127(02)00467-X)
7. K.D. Shepherd, M.G. Walsh. "Development of Reflectance Spectral Libraries for Characterization of Soil Properties". *Soil Sci. Soc. Am. J.* 2002. 66(3): 988–998. [10.2136/sssaj2002.9880](https://doi.org/10.2136/sssaj2002.9880)
8. R.A. Viscarra Rossel, T. Behrens, E. Ben-Dor, D.J. Brown, et al. "A Global Spectral Library to Characterize the World's Soil". *Earth-Sci. Rev.* 2016. 155: 198–230. [10.1016/j.earscirev.2016.01.012](https://doi.org/10.1016/j.earscirev.2016.01.012)
9. E. Ben Dor, N. Francos, Y. Ogen, A. Banin. "Aggregate Size Distribution of Arid and Semiarid Laboratory Soils (<2 mm) as Predicted by VIS-NIR-SWIR Spectroscopy". *Geoderma.* 2022. 416: 115819. [10.1016/j.geoderma.2022.115819](https://doi.org/10.1016/j.geoderma.2022.115819)
10. M.C. Sarathjith, B.S. Das, H.B. Vasava, B. Mohanty, et al. "Diffuse Reflectance Spectroscopic Approach for the Characterization of Soil Aggregate Size Distribution". *Soil Sci. Soc. Am. J.* 2014. 78(2): 369–376. [10.2136/sssaj2013.08.0377](https://doi.org/10.2136/sssaj2013.08.0377)
11. E. Ben-Dor, A. Banin. "Near-Infrared Analysis as a Rapid Method to Simultaneously Evaluate Several Soil Properties". *Soil Sci. Soc. Am. J.* 1995. 59(2): 364–372. [10.2136/sssaj1995.03615995005900020014x](https://doi.org/10.2136/sssaj1995.03615995005900020014x)
12. C.J. Bruegge, A.E. Stiegman, D.R. Coulter, R.R. Hale, et al. "Reflectance stability analysis of Spectralon diffuse calibration panels. Calibration of Passive Remote Observing Optical and Microwave Instrumentation". *Proceedings Volume 1493, Calibration of Passive Remote Observing Optical and Microwave Instrumentation.* 1991. Pp. 132–142. [10.1117/12.46691](https://doi.org/10.1117/12.46691)
13. A.R. Marjoram, P.J. Vickery, D.C. McKenzie. "A Polytetrafluoroethylene Coating for Field Reference Reflection

- Panels". *Int. J. Remote Sens.* 1990. 11(6): 1047–1053. [10.1080/01431169008955076](https://doi.org/10.1080/01431169008955076)
14. A. Springsteen. "Standards for Reflectance Measurements". In: J. Workman Jr., A. Springsteen, editors. *Applied Spectroscopy: A Compact Reference for Practitioners*. San Diego: Academic Press, 1998. Vol. 15, Pp. 247–267.
 15. J.D. Lindberg. "Absolute Diffuse Reflectance from Relative Reflectance Measurements". *Appl. Opt.* 1987. 26(14): 2900–2905. [10.1364/AO.26.002900](https://doi.org/10.1364/AO.26.002900)
 16. K. Elmer, R.J. Soffer, J.P. Arroyo-Mora, M. Kalacska. "ASDToolkit: A Novel Matlab Processing Toolbox for ASD Field Spectroscopy Data". *Data.* 2020. 5(4): 96. [10.3390/data5040096](https://doi.org/10.3390/data5040096)
 17. H.-R. Hannula, K. Heinilä, K. Böttcher, O.-P. Mattila, et al. "Laboratory, Field, Mast-Borne, and Airborne Spectral Reflectance Measurements of Boreal Landscape During Spring". *Earth Syst. Sci. Data.* 2020. 12(1): 719–740. [10.5194/essd-12-719-2020](https://doi.org/10.5194/essd-12-719-2020)
 18. K. Sakowska, D. Gianelle, A. Zaldej, A. MacArthur, et al. "WhiteRef: A New Tower-Based Hyperspectral System for Continuous Reflectance Measurements". *Sensors. Multidisciplinary Digital Publishing Institute*, 2015. 15(1): 1088–1105. [10.3390/s150101088](https://doi.org/10.3390/s150101088)
 19. R.J. Soffer, G. Ifimov, J.P. Arroyo-Mora, M. Kalacska. "Validation of Airborne Hyperspectral Imagery from Laboratory Panel Characterization to Image Quality Assessment: Implications for an Arctic Peatland Surrogate Simulation Site". *Can. J. Remote Sens.* 2019. 45(3–4): 476–508. [10.1080/07038992.2019.1650334](https://doi.org/10.1080/07038992.2019.1650334)
 20. E. Ben Dor, B. Efrati, O. Amir, N. Francos, et al. "A Standard and Protocol for In-Situ Measurement of Surface Soil Reflectance". *Geoderma.* 2024. 447: 116920. [10.1016/j.geoderma.2024.116920](https://doi.org/10.1016/j.geoderma.2024.116920)
 21. W. Möller, K.-P. Nikolaus, A. Höpe. "Degradation of the Diffuse Reflectance of Spectralon Under Low-Level Irradiation". *Metrologia.* 2003. 40(1): S212. [10.1088/0026-1394/40/1/349](https://doi.org/10.1088/0026-1394/40/1/349)
 22. A. Pimstein, G. Natesco, E. Ben-Dor. "Performance of Three Identical Spectrometers in Retrieving Soil Reflectance under Laboratory Conditions". *Soil Sci. Soc. Am. J.* 2011. 75(2): 746–759. [10.2136/sssaj2010.0174](https://doi.org/10.2136/sssaj2010.0174)
 23. A. Hueni, A. Damm, M. Kneubuehler, D. Schläpfer, M.E. Schaepman. "Field and Airborne Spectroscopy Cross Validation: Some Considerations". *IEEE J. Sel. Top. Appl. Earth Obs. Remote Sens.* 2017. 10(3): 1117–1135. [10.1109/JSTARS.2016.2593984](https://doi.org/10.1109/JSTARS.2016.2593984)
 24. E. Ben Dor, C. Ong, I.C. Lau. "Reflectance Measurements of Soils in the Laboratory: Standards and Protocols". *Geoderma.* 2015. 245–246: 112–124. [10.1016/j.geoderma.2015.01.002](https://doi.org/10.1016/j.geoderma.2015.01.002)
 25. E. Ben Dor, K. Karyotis, S. Chabrilat, T. Schmid. "Standardization and Protocol Development for Soil Spectral Reflectance in Laboratory and Field Settings: An Overview of IEEE SA P4005 Activity". *IGARSS 2024–2024 IEEE International Geoscience and Remote Sensing Symposium. Athens, Greece; 7–12 July 2024.* Pp. 268–270. [10.1109/IGARSS53475.2024.10641689](https://doi.org/10.1109/IGARSS53475.2024.10641689)
 26. V. Kopačková, E. Ben-Dor. "Normalizing Reflectance from Different Spectrometers and Protocols with an Internal Soil Standard". *Int. J. Remote Sens.* 2016. 37(6): 1276–1290. [10.1080/01431161.2016.1148291](https://doi.org/10.1080/01431161.2016.1148291)
 27. N. Francos, A. Gholizadeh, J.A.M. Demattê, E. Ben-Dor. "Effect of the Internal Soil Standard on the Spectral Assessment of Clay Content". *Geoderma.* 2022. 420: 115873. [10.1016/j.geoderma.2022.115873](https://doi.org/10.1016/j.geoderma.2022.115873)
 28. K. Karyotis, N.L. Tsakiridis, N. Tziolas, N. Samarinas, et al. "On-Site Soil Monitoring Using Photonics-Based Sensors and Historical Soil Spectral Libraries". *Remote Sens.* 2023. 15(6): 1624. [10.3390/rs15061624](https://doi.org/10.3390/rs15061624)
 29. E. Ben Dor, C. Ong, I.C. Lau. "Reflectance Measurements of Soils in the Laboratory: Standards and Protocols". *Geoderma.* 2015. 245–246: 112–124. [10.1016/j.geoderma.2015.01.002](https://doi.org/10.1016/j.geoderma.2015.01.002)
 30. N. Francos, E. Ben-Dor. "A Transfer Function to Predict Soil Surface Reflectance from Laboratory Soil Spectral Libraries". *Geoderma.* 2022. 405: 115432. [10.1016/j.geoderma.2021.115432](https://doi.org/10.1016/j.geoderma.2021.115432)
 31. J.A.M. Demattê, F. da Silva Terra. "Spectral Pedology: A New Perspective on Evaluation of Soils Along Pedogenetic Alterations". *Geoderma.* 2014. 217–218: 190–200. [10.1016/j.geoderma.2013.11.012](https://doi.org/10.1016/j.geoderma.2013.11.012)
 32. N. Richter, T. Jarmer, S. Chabrilat, C. Oyonarte, et al. "Free Iron Oxide Determination in Mediterranean Soils Using Diffuse Reflectance Spectroscopy". *Soil Sci. Soc. Am. J.* 2009. 73(1): 72–81. [10.2136/sssaj2008.0025](https://doi.org/10.2136/sssaj2008.0025)
 33. Malvern Panalytical. "Knowledge Center". <https://www.malvernpanalytical.com/en/learn/knowledge-center> [accessed 30 October 2025].
 34. G. Tóth, A. Jones, L. Montanarella. "The LUCAS Topsoil Database and Derived Information on the Regional Variability of Cropland Topsoil Properties in the European Union". *Environ. Monit. Assess.* 2013. 185(9): 7409–7425. [10.1007/s10661-013-3109-3](https://doi.org/10.1007/s10661-013-3109-3)
 35. J.A.M. Demattê, A.C. Dotto, A.F.S. Paiva, M.V. Sato, et al. "The Brazilian Soil Spectral Library (BSSL): A General View, Application, and Challenges". *Geoderma.* 2019. 354: 113793. [10.1016/j.geoderma.2019.05.043](https://doi.org/10.1016/j.geoderma.2019.05.043)
 36. E. Ben Dor, B. Efrati, O. Amir, N. Francos, et al. "A Standard and Protocol for In-Situ Measurement of Surface Soil Reflectance". *Geoderma.* 2024. 447: 116920. [10.1016/j.geoderma.2024.116920](https://doi.org/10.1016/j.geoderma.2024.116920)